


Spectra of a PH cycle

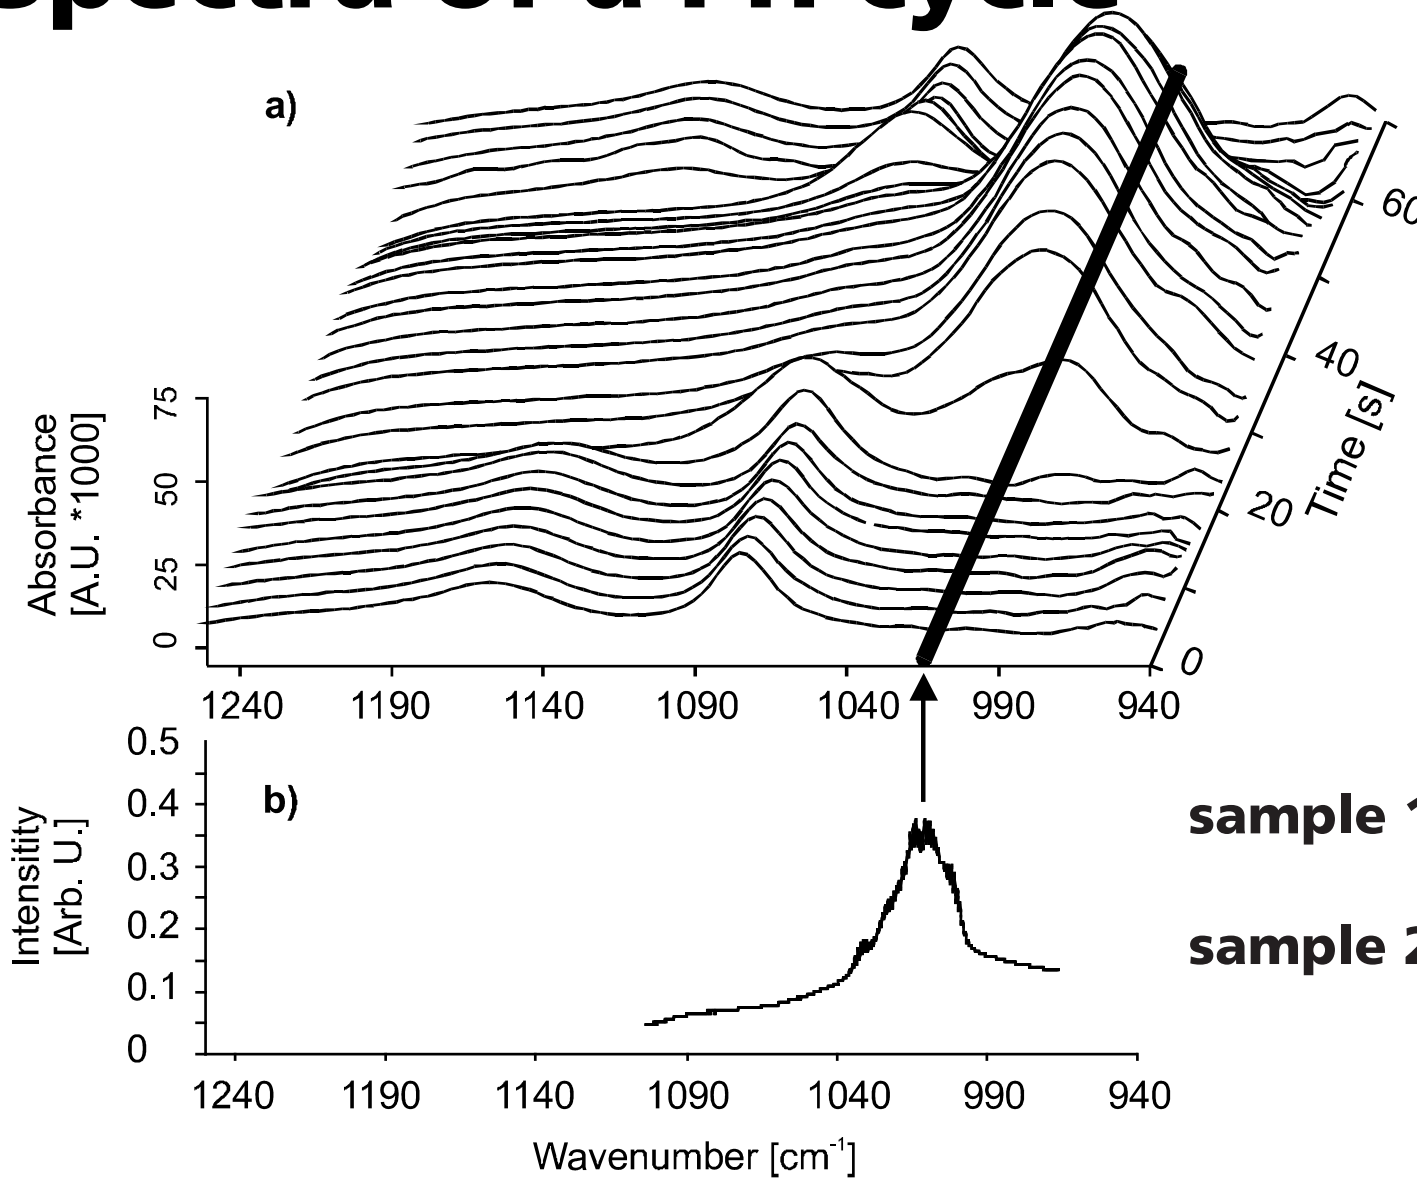

	QCL	ion chromatograph
sample 1	470 +/-10	478 +/-15
sample 2	530 +/-10	511 +/-15

Measurements in mg/l